



LuftBlick Report 2018013

## **Pandonia Operations**

Calibration results document

Version 10.0, 30<sup>th</sup> November 2020

	<b>Name</b>	<b>Company</b>
<b>prepared by</b>	Moritz Müller	LuftBlick
	Martin Tiefengraber	LuftBlick
	Manuel Gebetsberger	LuftBlick

## Contents

<b>Document Change Record</b>	<b>2</b>
<b>Acronyms and Abbreviations</b>	<b>3</b>
<b>1 Introduction</b>	<b>3</b>
1.1 Applicable Documents . . . . .	3
1.2 Reference Documents . . . . .	3
<b>2 Calibration overview</b>	<b>3</b>
2.1 Explanation . . . . .	3
2.2 Calibration frequency . . . . .	5
2.3 Calibrations foreseen between 1 <sup>st</sup> December and 28 <sup>th</sup> February . . . .	8
<b>A Calibration measurements in the laboratory</b>	<b>8</b>
<b>B Analysis of the laboratory measurements</b>	<b>8</b>
B.1 Field calibration . . . . .	8
B.2 Data quality checks . . . . .	9
<b>C Measurements with the mFCT</b>	<b>9</b>
<b>D Calibration towards a reference instrument</b>	<b>9</b>

## Document Change Record

Issue	Date	Section	Observations
0.1	26 <sup>th</sup> Nov 2018	All	First draft version
0.2	29 <sup>th</sup> Nov 2018	Summary	Adding software field calibration
2.0	30 <sup>th</sup> Nov 2018	All	Minor changes, first version 2
3.0	28 <sup>th</sup> Feb 2019	All	Minor changes, First version 3
4.0	27 <sup>th</sup> May 2019	Calibration frequency	Minor changes, First version 4
5.0	27 <sup>th</sup> Aug 2019	Calibration frequency	First version 5, updated figures and explanations, changes in section B.2
6.0	30 <sup>th</sup> Nov 2019	Update of figures section, minor changes in section B	
7.0	28 <sup>th</sup> Feb 2020	All	Update of figures and tables
8.0	31 <sup>st</sup> May 2020	All	Update of figures and tables
9.0	31 <sup>st</sup> August 2020	All	Update of figures and tables
10.0	30 <sup>th</sup> November 2020	All	Update of figures and tables

## Acronyms and Abbreviations

NO <sub>2</sub>	Nitrogene dioxide
O <sub>3</sub>	Ozone
FCS	Field Calibration Set
FRM4AQ	Fiducial Reference Measurements for Air Quality
ILB	Instrument Log Book
mFCT	Mobile Field Calibration Tool
MLE	Modified Langley Extrapolation
MobRef	Mobile Reference Pandora
PGN	Pandonia Global Network
rms	Root Mean Square
WP	Work Package

## 1 Introduction

This report is deliverable 6 (D6) of the ESA project “Pandonia Operations” (POp) [4, 5] and covers the last quarter from 1<sup>st</sup> September to 30<sup>th</sup> November 2020. Further, it provides an overview about calibration activities of Pandora instruments from the beginning of 2018 and an outlook of calibration activities for the next quarter.

### 1.1 Applicable Documents

- [1] CCN1 to ESA Ground-based Air-Quality Spectrometer Validation Network Uncertainties Study [Proposal, Proposal 201705A, Issue 2, 2017.
- [2] CCN1 to ESA Ground-Based Air-Quality Spectrometer Validation Network and Uncertainties Study [Statement of Work], ESA-EOPG- MOM-SOW-1, Issue 1, Revision 1, 2017.
- [3] Fiducial Reference Measurements for Air Quality [Statemet of Work], ESA ESA-EOPG-MOM-SOW-0046, Issue 1, Revision 5, 2018.
- [4] Pandonia Operations [Proposal], LuftBlick Proposal 201804OPE, Issue 1, 2018.

[5] Pandonia Operations [Contract and Statement of Work], ESA Contract No. 4000124223/18/I-SBo, 2018.

[7] J. Herman, A. Cede, E. Spinei, G. Mount, M. Tzortziou, and N. Abuhassan. NO<sub>2</sub> column amounts from ground-based Pandora and MFDOAS spectrometers using the direct-sun DOAS technique: Intercomparisons and application to OMI validation. *Journal of Geophysical Research (Atmospheres)*, 114:D13307, July 2009. doi: 10.1029/2009JD011848.

## 1.2 Reference Documents

[7] J. Herman, A. Cede, E. Spinei, G. Mount, M. Tzortziou, and N. Abuhassan. NO<sub>2</sub> column amounts from ground-based Pandora and MFDOAS spectrometers using the direct-sun DOAS technique: Intercomparisons and application to OMI validation. *Journal of Geophysical Research (Atmospheres)*, 114:D13307, July 2009. doi: 10.1029/2009JD011848.

## 2 Calibration overview

### 2.1 Explanation

Explanation of the figures which are shown on the next two pages:

- **Lab** stands for laboratory, **Fld** for field, **Ana** for analysis, **Haw** for hardware and **Ref** for reference.
- **HawLab** means measurements in the laboratory in order to determine instrument specific characteristics, more information is given in section A.
- **AnaLab** is the analysis of the measurements taken in the laboratory (details are provided in section B).
- **AnaFld** is a field calibration where solar based L0 data and L1 data are used, for more information refer to section B.1.
- **HawFld** is a field calibration where measurements are done with the mobile field calibration tool mFCT, further information is given in section C.

- **RefFld** denotes the visit of the field calibration set FCS, for details go to section D.

All Pandoras, official PGN and non-official PGN Pandora instruments are taken into account.

All finished laboratory measurements are listed in the figures, this means no sessions which had to be redone (explained further in A). For analysis sessions, only calibration sessions are listed which have been finished and data has been processed with these calibrations (B). Measurements with the mFCT and calibrations towards a planned mobile reference instrument are also shown for completeness.

## 2.2 Calibration frequency



In the last quarter, a lot of laboratory calibrations have been done at SciGlob and NASA. Many new instruments are built at the moment and NASA opened after the COVID-19 shutdown, so many instruments have been in the pipeline to be upgraded and calibrated at NASA. Since many instruments have been built, a lot of field clearing had to be done, meaning the calibration team had to go sure that the data of the new or upgraded instruments is good and the instruments are ready for shipping. The main focus of the calibration analysis work is still the instruments delivering data for satellite validation but further, a significant number of old campaign datasets have been recalibrated and reprocessed. Note that we still want to have all datasets calibrated and processed with Blick 1.7, so that we have a homogenized dataset.

We typically split up the work that NASA staff is doing the calibration work of the instruments from NASA and EPA and LuftBlick is doing the European instruments. But since the calibration analysis team in the USA consists of just one person, LuftBlick has to help out with analysis of the laboratory data. But, on the other hand, LuftBlick gets support with laboratory calibrations (e.g. P105; straylight calibration).

**Figure 1:** Calibration activities

(a) 1<sup>st</sup> September 2020 to 30<sup>th</sup> November 2020

(b) 1<sup>st</sup> January 2018 to 30<sup>th</sup> November 2020.

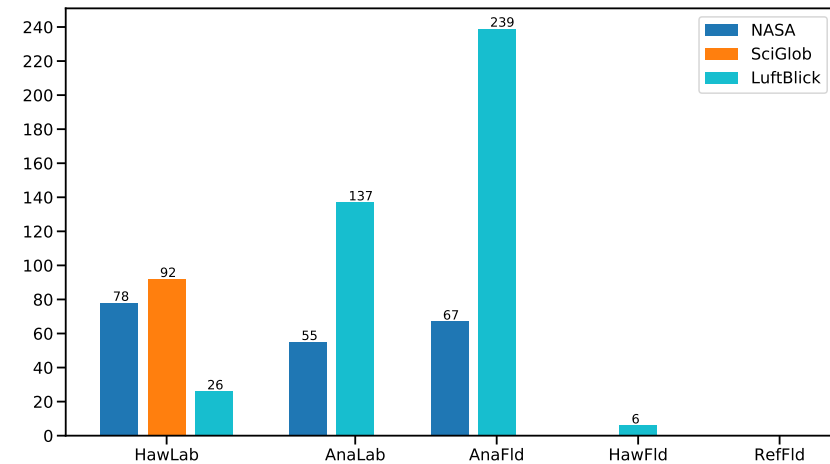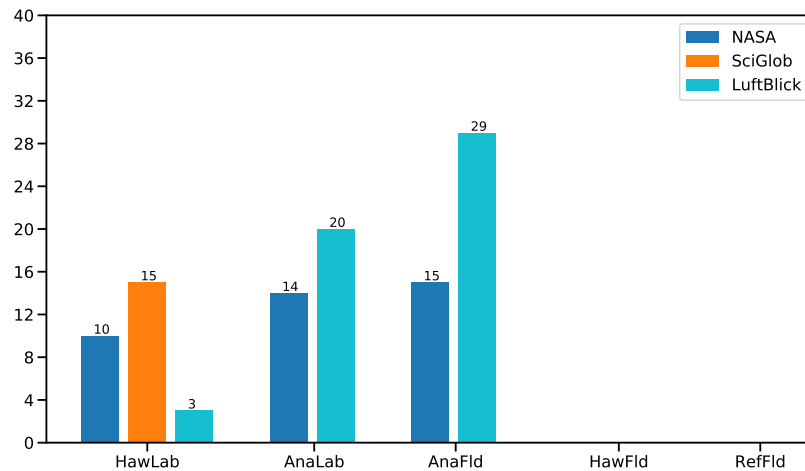

A detailed list of the calibration analysis work for the last quarter. A lot of clearing instruments are listed which means, instruments at the testing locations have been calibrated to ensure a good data quality before shipping the instrument to its final location. E.g. P146 in Yokosuka has two calibrations, one field clearing for ElkridgeMD, i.e. the testing location and a further field calibration for Yokosuka. Field clearing locations are typically ElkridgeMD, GreenbeltMD and Innsbruck-FKS.

<b>Instrument ID</b>	<b>Location</b>	<b>Nr. of AnaFld</b>	<b>Purpose</b>
2 - UV	GreenbeltMD	1	New field calibration
20 - UV	GreenbeltMD	1	Field clearing
26 - UV	GreenbeltMD	1	Field clearing
31 - UV	CharlesCityVA	1	Updated field calibration after one year
34 - UV	BoulderCO	3	Recalibration of old dataset (2013-2017)
39 - UV	GreenbeltMD	1	Field clearing
49 - UV	GreenbeltMD	1	Field clearing
54 - UV	GreenbeltMD	1	Field clearing
56 - UV	MaunaLoaHI, New-BrunswickNJ	2	Field calibration for MaunaLoaHI data and re-calibration of old NewBrunswickNJ dataset
58 - UV	GreenbeltMD	1	Field clearing
65 - UV	GreenbeltMD	1	Field clearing
105 - UV	Helsinki	1	Field calibration of latest validity period
111 - UV	Bucharest	1	New field calibration to have good live data
117 - UV	Rome-SAP	4	Recalibration of whole dataset

<b>Instrument ID</b>	<b>Location</b>	<b>Nr. of AnaFld</b>	<b>Purpose</b>
118 - UV	Cabauw	1	Field calibration
119 - UV	Innsbruck-FKS	1	Field clearing
120 - UV	Davos	1	New field calibration to have good live data
126 - UV	Innsbruck-FKS	1	Field clearing
132 - UV	Innsbruck-FKS	1	Field clearing
138 - UV	Rome-SAP, Rome-IIA	2	New field calibrations of the two locations
140 - UV	WashingtonDC	1	Field calibration
142 - UV	ElkridgeMD	1	Field clearing
146 - UV	ElkridgeMD, Yokosuka	2	Field clearing and new field calibration for Yokosuka
149 - UV	ElkridgeMD, SeoulSNU	2	Field clearing and new field calibration for SeoulSNU
150 - UV	Ulsan	1	New field calibration
161 - UV	ElkridgeMD	1	Field clearing
164 - UV	ElkridgeMD, SeoulSNU	3	Field clearing and new field calibrations for SeoulSNU
176 - UV	ElkridgeMD	1	Field clearing
177 - UV	GreenbeltMD, ElkridgeMD	2	Field clearing
178 - UV	ElkridgeMD	1	Field clearing
180 - UV	GreenbeltMD	1	Field clearing
181 - UV	SanJoseCA	1	New field calibration

## 2.3 Calibrations foreseen between 1<sup>st</sup> December and 28<sup>th</sup> February

The main calibration tasks in the next quarter:

1. The weekly data quality checks will raise our attention to instruments which are having data quality issues, i.e. they need a new field calibration. This has highest priority for instruments being used for satellite validation, to assure best data quality on a continuous basis
2. Field clearing instruments
3. Continue with the recalibration of older datasets to have a homogenized database

Calibration activity	Expected number	Details
HawLab	> 6	Initial calibrations by NASA & SciGlob, in Innsbruck it is planned to re-calibrate P106 and P121
AnaLab	> 10	Field clearance for instruments which are measured in the laboratory soon. Recalibration of old datasets.
AnaFld	> 10	Field calibrations for the instruments mentioned in AnaLab
HawFld	-	-
RefFld	-	-

## A Calibration measurements in the laboratory

The first step after the assembling of an instrument is the initial calibration in a laboratory. Currently, three institutions are doing laboratory measurements of the Pandora spectrometer system:

- SciGlob

- NASA
- LuftBlick.

Before shipping an instrument after the initial calibration, the measurements are checked by LuftBlick. Some of the measurements have to be redone since they are not of best possible quality. An example would be bad alignment of the calibration lamp or an unstable laboratory setup. Another case, in which laboratory measurements have to be redone, is the situation that an instrument does not work properly during the field testing period and repair work has to be done. Then, a new laboratory session is performed. The numbers in the overview figures in section 2 do not include laboratory sessions which had to be re-done because of the mentioned reasons. So, the number of laboratory measurements in the figures 1b and 1a can be lower than the actual number of laboratory sessions. One full calibration, without unpacking, installing and testing the instrument lasts about 2.5 days. This includes dark signal and wavelength calibration at three different temperatures in order to determine the temperature dependence of these two properties.

## B Analysis of the laboratory measurements

Since the workshop in May 2019 in Innsbruck, when three NASA colleagues and one EPA colleague have been taught in the analysis of laboratory measurements, LuftBlick gets support with the calibration work. In the NASA team just two people are working on the analysis of laboratory data anymore. To keep the NASA and EPA colleagues informed about changes in the calibration procedures and to calibrate the instruments in a homogenous way, regular telecons are held and individual support is given by LuftBlick. Although the BlickC is a semi-automated software, still some experience is needed to operate it and to finally produce a proper calibration analysis. As always, in the overview figures in section 2, just analysis sessions are shown which have finally been pushed on the server and are being used for data processing. This means it is either under live processing or on EVDC.

### B.1 Field calibration

A crucial part of the calibration procedure for Pandoras is the field calibration. Part of this step is to detect a possible change in the spectral dispersion (wavelength



shift). Such changes might appear e.g. during the shipping of the instrument or if the fiber is unplugged. Furthermore, for NO<sub>2</sub>, a reference is created from Pandoras own measurements and a MLE (explained in [7]), is done in the field calibration. For this MLE we need some weeks or even months of field measurements, depending on the location and weather conditions.

So, new field calibrations are necessary for the following scenarios:

- Initial calibration of an instrument.
- If there is a jump in the data quality parameters (e.g. wrms or wavelength shift) which can e.g. come from repairing works or location changes.
- When the data quality exceeds certain thresholds which will be determined by the rMLE (explained in detail in B.2).

The amount of field calibrations is relatively high at the moment since we are re-calibrating and re-processing the datasets.

## B.2 Data quality checks

In order to have continuous data quality checks, the final NO<sub>2</sub> and O<sub>3</sub> total column data is checked manually. Different data quality parameters and the total column amounts of NO<sub>2</sub> and O<sub>3</sub> are taken into account. Right now, these checks are mainly done offline. Whole timeseries are checked, i.e. the data of the whole time period when an instrument was operational (timeseries go up to now if it is still operational), is processed and checked manually. Therefore, data quality parameters are taken into account which give information about changes in the instrument. An example would be that the fiber gets unplugged, because it is impossible to plug it in again exactly the same way and the instrument is slightly different than it has been before. This can be seen in the wavelength shift and the rms. An information about the quality of the alignment is given in the uncertainty. Mainly these three parameters, together with the final data, are screened for magnitude and jumps. Sometimes it can be the case that these parameters are not enough and we take all information given in the data files and from the ILB to evaluate the data quality. If an instrument gets an initial calibration, we have an idea about the order of magnitude of these quality parameters at a certain location. If there is a significant jump in one of these parameters, we have already a good reason for a new calibration since something

changed in the instrument. In combination with the information about the instrument performance from the ILB, this is used for detecting when a new calibration has to be done to have highest data quality possible. Most of it is currently done offline, but the live visualization is already used to detect these data jumps as well. The long term plan is to base the decision, of when a new calibration has to be done, on what is seen in the live visualization. With this tool, Pandoras, which need a new calibration can immediately be detected.

In the FRM4AQ project, WP4 (refer to [3]) this and other QA/QC procedures will be further studied and refined.

## C Measurements with the mFCT

In WP 2 of the Pandonia CCN project [1] [2], a mFCT has been developed. The idea is to track changes of the instrument without the need to dismount and ship it to a laboratory. For the following scenarios, measurements with the mFCT will be done:

- After hardware changes and other repair work on the instrument.
- After actions on the instrument like unplugging the fiber or dismounting the instrument, in order to keep track of changes of the spectral response and to update the absolute calibration.
- After a long period of time in order to track changes and degradation of the hardware, e.g. of the filters.

## D Calibration towards a reference instrument

The network strategy foresees a FCS which consists of the mFCT and a MobRef. For details refer to [4]. The acquisition of a MobRef through FRM4AQ is planned for 2021. Actions with the FCS will be done and listed in this report as soon as it is operationally utilized.